

# Cerebral Oxygenation during Laparoscopic Surgery: Jugular Bulb versus Regional Cerebral Oxygen Saturation

Seung Ho Choi,<sup>1</sup> Soo Hwan Kim,<sup>2</sup> Sung Jin Lee,<sup>1</sup> Sa Rah Soh,<sup>1</sup> and Young Jun Oh<sup>1</sup>

<sup>1</sup>Department of Anesthesiology and Pain Medicine, Anesthesia and Pain Research Institute, Yonsei University College of Medicine, Seoul;

<sup>2</sup>Department of Anesthesiology and Pain Medicine, Kangnam Sacred Heart Hospital, Hallym University College of Medicine, Seoul, Korea.

Received: December 21, 2011

Revised: February 6, 2012

Accepted: February 24, 2012

Corresponding author: Dr. Young Jun Oh,  
Department of Anesthesiology and  
Pain Medicine, Anesthesia and  
Pain Research Institute,  
Yonsei University College of Medicine,  
50 Yonsei-ro, Seodaemun-gu,  
Seoul 120-752, Korea.  
Tel: 82-2-2228-2423, Fax: 82-2-312-7185  
E-mail: yjoh@yuhs.ac

The authors have no financial conflicts of interest.

**Purpose:** We hypothesized that regional cerebral oxygen saturation (rSO<sub>2</sub>) could replace jugular bulb oxygen saturation (SjvO<sub>2</sub>) in the steep Trendelenburg position under pneumoperitoneum. Therefore, we evaluated the relationship between SjvO<sub>2</sub> and rSO<sub>2</sub> during laparoscopic surgery. **Materials and Methods:** After induction of anesthesia, mechanical ventilation was controlled to increase PaCO<sub>2</sub> from 35 to 45 mm Hg in the supine position, and the changes in SjvO<sub>2</sub> and rSO<sub>2</sub> were measured. Then, after establishment of pneumoperitoneum and Trendelenburg position, ventilation was controlled to maintain a PaCO<sub>2</sub> at 35 mm Hg and the CO<sub>2</sub> step and measurements were repeated. The changes in SjvO<sub>2</sub> (rSO<sub>2</sub>)-CO<sub>2</sub> reactivity were compared in the supine position and Trendelenburg-pneumoperitoneum condition, respectively. **Results:** There was little correlation between SjvO<sub>2</sub> and rSO<sub>2</sub> in the supine position (concordance correlation coefficient=0.2819). Bland-Altman plots showed a mean bias of 8.4% with a limit of agreement of 21.6% and -4.7%. SjvO<sub>2</sub> and rSO<sub>2</sub> were not correlated during Trendelenburg-pneumoperitoneum condition (concordance correlation coefficient=0.3657). Bland-Altman plots showed a mean bias of 10.6% with a limit of agreement of 23.6% and -2.4%. The SjvO<sub>2</sub>-CO<sub>2</sub> reactivity was higher than rSO<sub>2</sub>-CO<sub>2</sub> reactivity in the supine position and Trendelenburg-pneumoperitoneum condition, respectively (0.9±1.1 vs. 0.4±1.2% mm Hg<sup>-1</sup>, *p*=0.04; 1.7±1.3 vs. 0.5±1.1% mm Hg<sup>-1</sup>, *p*<0.001). **Conclusion:** There is little correlation between SjvO<sub>2</sub> and rSO<sub>2</sub> in the supine position and Trendelenburg-pneumoperitoneum condition during laparoscopic surgery.

**Key Words:** Cerebral oxygenation, jugular bulb oxygen saturation, laparoscopy, pneumoperitoneum

## INTRODUCTION

Lower abdominal laparoscopic surgery often requires the patient to be placed in a steep Trendelenburg position in order to secure a clear surgical field.<sup>1</sup> However, when this position is combined with CO<sub>2</sub> pneumoperitoneum, the risk of potential changes in cerebral hemodynamics such as an increase in cerebral blood flow (CBF) is increased.<sup>2,3</sup>

Jugular bulb oxygen saturation (SjvO<sub>2</sub>) reflects the relationship between global

### © Copyright:

Yonsei University College of Medicine 2013

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

cerebral oxygen supply and demand. Provided that the cerebral metabolic rate is constant, S<sub>ijv</sub>O<sub>2</sub> is a useful indicator of CBF.<sup>4,5</sup> However, jugular bulb catheterization is an invasive procedure and has inherent potential complications such as bleeding and nerve damage. Near-infrared spectroscopy is a monitoring device for non-invasive assessment of regional cerebral oxygen saturation (rSO<sub>2</sub>).<sup>4,6</sup> It is widely used in patients undergoing various procedures because real-time information is provided non-invasively.<sup>7,8</sup> Previous studies evaluated the agreement between S<sub>ijv</sub>O<sub>2</sub> and rSO<sub>2</sub> with contradictory results in various situations.<sup>9-11</sup> To our knowledge, the relationship between S<sub>ijv</sub>O<sub>2</sub> and rSO<sub>2</sub> in the supine and Trendelenburg-pneumoperitoneum condition has not been investigated. In this study, we hypothesized that rSO<sub>2</sub> could reflect S<sub>ijv</sub>O<sub>2</sub> in the steep Trendelenburg position under pneumoperitoneum. Therefore, we evaluated the relationship between S<sub>ijv</sub>O<sub>2</sub> and rSO<sub>2</sub> during laparoscopic surgery.

## MATERIALS AND METHODS

After Institutional Review Board approval and the acquisition of written informed consent, 35 consecutive male patients scheduled for robot-assisted laparoscopic radical prostatectomy were enrolled in this study. Patients with neurological diseases, a history of carotid artery stenosis or transient ischemic attack were excluded.

### Conduct of anesthesia and monitoring

No premedication was given. Continuous electrocardiography and pulse oximetry monitoring was done upon arrival at the operating room. General anesthesia was induced according to a standardized regimen of intravenous propofol 1.5 mg·kg<sup>-1</sup>, remifentanyl 1 µg·kg<sup>-1</sup> and rocuronium 0.6 mg·kg<sup>-1</sup>. After endotracheal intubation, the lungs were ventilated with 50% oxygen. Anesthesia was maintained with 1 minimum alveolar concentration end-tidal concentration of sevoflurane and remifentanyl infusion of 0.1-0.2 µg·kg<sup>-1</sup>·min<sup>-1</sup>. A 20-G catheter was inserted in the radial artery for arterial blood pressure monitoring and arterial blood gas analysis. Mechanical ventilation was done with a tidal volume of 8-10 mL·kg<sup>-1</sup> to maintain PaCO<sub>2</sub> at 35 mm Hg, and the concordance between PaCO<sub>2</sub> and end-tidal CO<sub>2</sub> tension was measured. A bispectral index score (BIS) monitor (A-2000 BIS Monitor™, Aspect Medical System Inc., Newton, MA, USA) was monitored continuously to maintain appropriate anesthetic depth during the procedure.

For S<sub>ijv</sub>O<sub>2</sub> measurement, a 4-F dual oximeter catheter™ (Edwards Lifesciences, Irvine, CA, USA) was inserted into the left internal jugular vein according to the modified Seldinger technique. When resistance was sensed during advancement in the cephalad direction, the catheter was withdrawn about 1-2 mm and the position of the jugular bulb catheter tip was immediately confirmed radiographically. The ideal catheter tip position is cranial to the line extending from the atlanto-occipital joint space, and caudal to the lower margin of the orbit. Once correct position was confirmed, the catheter was connected to the monitor (CCOmbO/SvO<sub>2</sub> Model 744HF75™, Baxter Healthcare Corporation, Irvine, CA, USA) for continuous S<sub>ijv</sub>O<sub>2</sub> monitoring and *in vivo* calibration was done by drawing a blood sample from the catheter. For rSO<sub>2</sub> measurement, sensors for cerebral oximetry were placed bilaterally at least 2 cm above the eyebrow on both sides of the forehead. The rSO<sub>2</sub> value was continuously monitored using near-infrared spectroscopy (INVOS 5100™, Somanetics Corp., Troy, MI, USA). Body temperature was maintained at 36.0-37.0°C by applying a forced-air warming system (Bair-Hugger™, Augustine-Medical, Eden Prairie, MN, USA) as needed.

### Conduct of the study and measurements

After induction of anesthesia, blood gases, S<sub>ijv</sub>O<sub>2</sub>, rSO<sub>2</sub>, mean arterial pressure, heart rate and BIS were all measured in the supine position with PaCO<sub>2</sub> maintained at 35 mm Hg for 10 min (T<sub>1</sub>). Mechanical ventilation was then adjusted to increase PaCO<sub>2</sub> to 45 mm Hg for 10 min, and all measurements were repeated (T<sub>2</sub>). After the patient was placed in a 30° Trendelenburg position and CO<sub>2</sub> pneumoperitoneum was established (intra-abdominal pressure <18 mm Hg), ventilation was controlled to maintain PaCO<sub>2</sub> at 35 mm Hg for 10 min and all measurements were repeated (T<sub>3</sub>). Ventilation was adjusted once more to increase and maintain PaCO<sub>2</sub> at 45 mm Hg for 10 min, and all measurements were repeated (T<sub>4</sub>).

At each 30 second point in time, the rSO<sub>2</sub> values from both sides recorded during blood sampling were averaged for the same time at which the blood sample for the S<sub>ijv</sub>O<sub>2</sub> measurement was drawn.

### Statistical analysis

The data are presented as means (SD) or range. We used a concordance correlation coefficient (CCC) to evaluate the agreement between S<sub>ijv</sub>O<sub>2</sub> and rSO<sub>2</sub>.<sup>12</sup> The CCC covers components of both precision (degree of variation) and ac-

curacy (degree of location or scale shift), thus providing sound intuitive interpretations. Ranging from 0 to 1, higher values of CCC indicate more concordant data. Bland-Altman analysis was done to determine the magnitude of the difference between two measurements.<sup>13</sup> Based on a previous study,<sup>9</sup> we postulated that a difference of 5% between the two parameters would be clinically acceptable under the hypothesis that the two methods are interchangeable. All data were analyzed using MedCalc software 9.3.6.0 (MedCalc Inc., Mariakerke, Belgium).

We also compared the change in S<sub>ijv</sub>O<sub>2</sub> (or rSO<sub>2</sub>) -CO<sub>2</sub> reactivity in the supine position and Trendelenburg-pneumoperitoneum condition. The S<sub>ijv</sub>O<sub>2</sub> (or rSO<sub>2</sub>) -CO<sub>2</sub> reactivity was defined as the % change in S<sub>ijv</sub>O<sub>2</sub> (or rSO<sub>2</sub>) by the step change induced in PaCO<sub>2</sub>. Comparison of the reactivity values of S<sub>ijv</sub>O<sub>2</sub> (or rSO<sub>2</sub>) -CO<sub>2</sub> calculated in the supine position and Trendelenburg-pneumoperitoneum condition were done using the paired t-test. Analysis of other intraoperative variables at each time period was done with repeated measures ANOVA. Data were analyzed using SPSS version 13.0 (SPSS Inc., Chicago, IL, USA). A *p* value <0.05 was considered statistically significant.

## RESULTS

Patients' characteristics and operation data are summarized in Table 1.

Measurements of the cerebral oxygen profiles and hemodynamic variables during study periods are listed in Table 2.

**Table 2. Measurements of the Cerebral Oxygen Profiles and Hemodynamic Variables during Study Periods**

	T <sub>1</sub>	T <sub>2</sub>	T <sub>3</sub>	T <sub>4</sub>
S <sub>ijv</sub> O <sub>2</sub> (%)	74.2±4.9	81.0±7.5 <sup>†</sup>	72.6±7.1	84.0±7.5 <sup>‡</sup>
rSO <sub>2</sub> (%)	68.1±5.3	70.3±7.1	66.1±6.1	69.3±7.7
MAP (mm Hg)	83.1±10.2	85.1±13.2	92.2±10.1*	88.8±11.2
HR (beats·min <sup>-1</sup> )	64.3±12.9	65.6±10.4	69.4±9.5	67.5±14.8

S<sub>ijv</sub>O<sub>2</sub>, jugular bulb oxygen saturation; rSO<sub>2</sub>, regional cerebral oxygen saturation; MAP, mean arterial pressure; HR, heart rate.

Values are mean±SD. T<sub>1</sub> and T<sub>2</sub>, PaCO<sub>2</sub> of 35 and 45 mm Hg in supine position, respectively; T<sub>3</sub> and T<sub>4</sub>, PaCO<sub>2</sub> of 35 and 45 mm Hg in the Trendelenburg position under pneumoperitoneum, respectively.

\**p*<0.05 and <sup>†</sup>*p*<0.001 compared with the value at T<sub>1</sub>.

<sup>‡</sup>*p*<0.001 compared with the value at T<sub>3</sub>.

**Table 3. The Relationship between Jugular Bulb Oxygen Saturation and Regional Cerebral Oxygen Saturation during Study Periods**

	Supine	Trendelenburg-pneumoperitoneum
Concordance correlation coefficient	0.2819	0.3657
95% confidence interval	0.1527-0.4017	0.2492-0.4718
Precision (Pearson's ρ)	0.5104	0.6977
Accuracy (Bias correction factor)	0.5523	0.5241

S<sub>ijv</sub>O<sub>2</sub> values ranged from 59.0 to 92.7% whereas the values for rSO<sub>2</sub> ranged from 52 to 88% during study periods. Cerebral oxygen saturation as measured by rSO<sub>2</sub> was about 12% lower than that measured by S<sub>ijv</sub>O<sub>2</sub>. With an increase of PaCO<sub>2</sub>, S<sub>ijv</sub>O<sub>2</sub> increased significantly both in the supine and Trendelenburg position (*p*<0.001).


Seventy comparative measurements were performed between S<sub>ijv</sub>O<sub>2</sub> and rSO<sub>2</sub> in the supine position and Trendelenburg-pneumoperitoneum condition, respectively. There was little correlation between S<sub>ijv</sub>O<sub>2</sub> and rSO<sub>2</sub> in the supine position (concordance correlation coefficient=0.2819) (Table 3) (Fig. 1A). Bland-Altman plots showed a mean bias of 8.4% with a limit of agreement of 21.6% and -4.7% (Fig. 1B). In addition, S<sub>ijv</sub>O<sub>2</sub> and rSO<sub>2</sub> were not correlated during Trendelenburg-pneumoperitoneum condition (concordance correlation coefficient=0.3657) (Table 3) (Fig. 2A). Bland-Altman plots showed a mean bias of 10.6% with a limit of agreement of 23.6% and -2.4% (Fig. 2B).

The S<sub>ijv</sub>O<sub>2</sub>-CO<sub>2</sub> reactivity was higher than rSO<sub>2</sub>-CO<sub>2</sub> reactivity in the supine position and Trendelenburg-pneumoperitoneum condition, respectively (0.9±1.1 vs. 0.4±1.2%·mm


**Table 1. Patients' Characteristics and Operation Data**

	n=35
Age (yrs)	61.7±11.0 (43-72)
Height (cm)	166.4±4.9 (158-175)
Weight (kg)	65.9±8.3 (53-81)
Body mass index (kg·m <sup>-2</sup> )	23.7±2.5 (19.6-29.4)
Duration of operation time (min)	176±22
Duration of pneumoperitoneum (min)	142±24

Values are mean±SD (range) or number of patients.

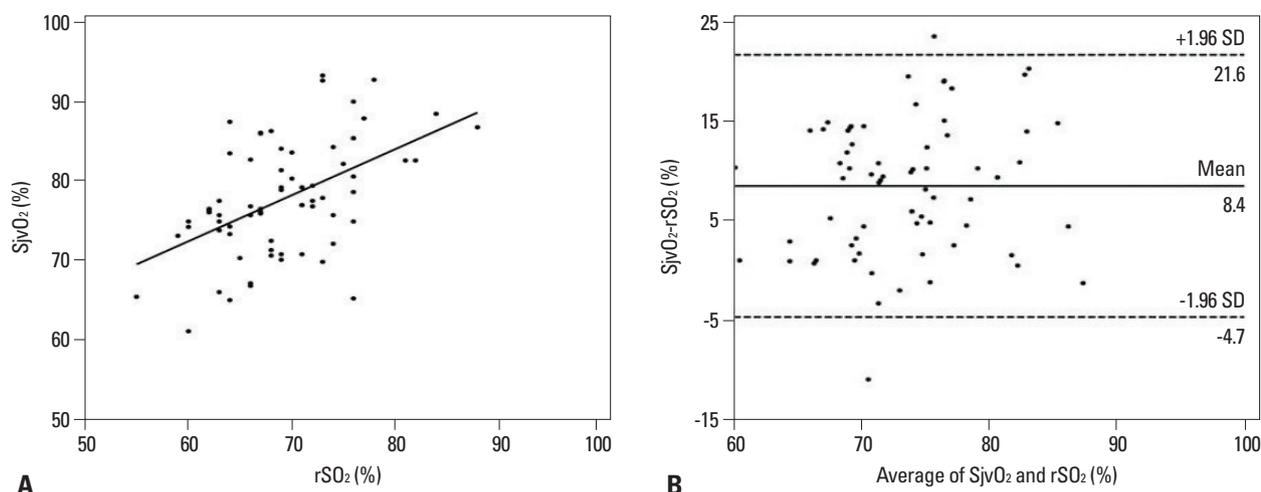

**Fig. 1.** Concordance correlation (A) and Bland-Altman analysis (B) of the measured difference between jugular bulb oxygen saturation (SjvO<sub>2</sub>) and regional cerebral oxygen saturation (rSO<sub>2</sub>) in the supine position.

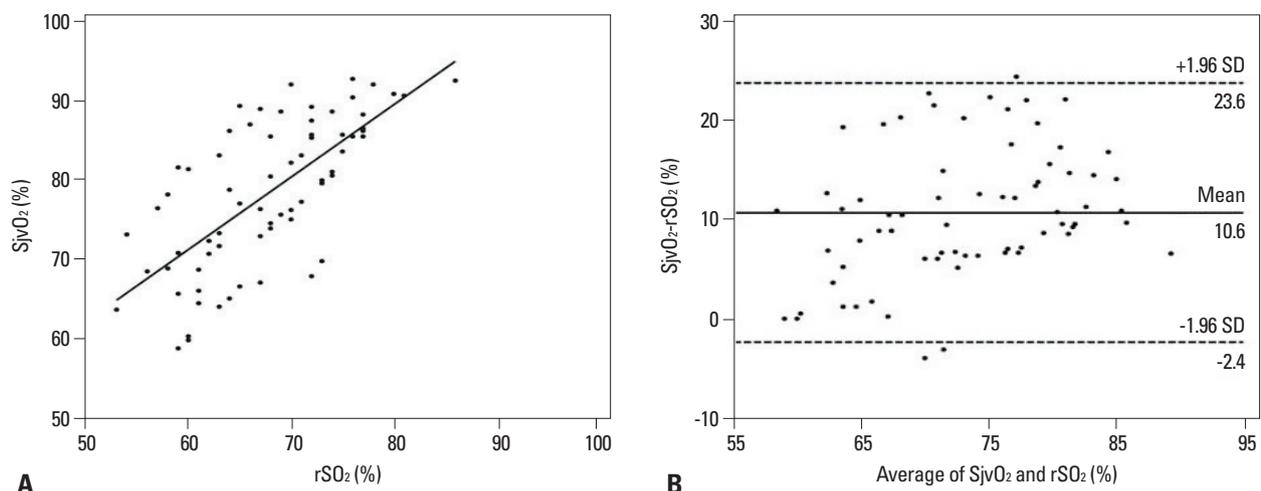

**Fig. 2.** Concordance correlation (A) and Bland-Altman analysis (B) of the measured difference between jugular bulb oxygen saturation (SjvO<sub>2</sub>) and regional cerebral oxygen saturation (rSO<sub>2</sub>) in the Trendelenburg-pneumoperitoneum condition.

Hg<sup>-1</sup>,  $p=0.04$ ;  $1.7\pm 1.3$  vs.  $0.5\pm 1.1\%$ ·mm Hg<sup>-1</sup>,  $p<0.001$ ). The SjvO<sub>2</sub>-CO<sub>2</sub> reactivity was higher in the Trendelenburg-pneumoperitoneum condition compared to the supine position ( $1.7\pm 1.3$  vs.  $0.9\pm 1.1\%$ ·mm Hg<sup>-1</sup>,  $p<0.001$ ). No adverse effects related to jugular venous catheterization were observed.

## DISCUSSION

Our main result is that there is little correlation between SjvO<sub>2</sub> and rSO<sub>2</sub> in the supine position and Trendelenburg-pneumoperitoneum condition during laparoscopic surgery. Although episodes of clinically significant cerebral desaturation were not detected in this clinical setting, Bland-Altman analysis demonstrated that both rSO<sub>2</sub> and SjvO<sub>2</sub> are not interchangeable values in this study.

There are some studies investigating the correlation between rSO<sub>2</sub> and SjvO<sub>2</sub> under specific clinical situations with contrary results. Kim, et al.<sup>14</sup> reported good agreement between rSO<sub>2</sub> and SjvO<sub>2</sub> measurements in healthy volunteers during isocapnic hypoxia. However, Leyvi, et al.<sup>10</sup> demonstrated that there was only a weak correlation between rSO<sub>2</sub> and SjvO<sub>2</sub>, and individual variation was wide during deep hypothermic circulatory arrest. Nagdyman, et al.<sup>9</sup> reported that rSO<sub>2</sub> demonstrated a substantial bias of the measurements to SjvO<sub>2</sub> in children with congenital heart disease, which is in agreement with our results. In our study, there was poor agreement, significant bias, and imprecision between SjvO<sub>2</sub> and rSO<sub>2</sub> in the supine position and Trendelenburg-pneumoperitoneum condition during laparoscopic surgery.

The disagreement between SjvO<sub>2</sub> and rSO<sub>2</sub> may be attributed to several factors. First, there is a significant differ-

ence in measuring cerebral oxygen saturation between  $SjvO_2$  and  $rSO_2$ .  $rSO_2$  measures cerebral oxygen saturation in a small region of the brain and may be influenced by blood distribution or signals caused by extracerebral tissues,<sup>15,16</sup> and  $SjvO_2$  represents global cerebral oxygen saturation. Furthermore, Knirsch, et al.<sup>17</sup> demonstrated that  $rSO_2$  correlates better with central venous oxygen saturation than  $SjvO_2$ .  $rSO_2$  is influenced by both cerebral and extracerebral components; therefore, the impact of extracerebral components on the  $rSO_2$  reading should not be underestimated. In our study, cerebral oxygen saturation as measured by  $rSO_2$  was about 12% lower than that measured by  $SjvO_2$ . Also, changes in extracerebral blood flow, variation in inter-individual absorption differences and changed position of the probes over time may affect the measurements of  $rSO_2$ .<sup>18,19</sup>

Body position and  $PaCO_2$  can also influence cerebral oxygen saturation. A previous study demonstrated that  $rSO_2$  was decreased in association with the Trendelenburg position and was further impaired by hypercapnia and pneumoperitoneum during laparoscopic surgery.<sup>20</sup> Another study demonstrated that  $rSO_2$  increased during Trendelenburg-pneumoperitoneum condition and  $PaCO_2$  increased in a similar manner,<sup>21</sup> which is in accordance with our study. In this study, an increase of  $PaCO_2$  also increased  $SjvO_2$  significantly both in the supine and Trendelenburg position, and  $rSO_2$  increased slightly in this period. Therefore, it is suggested that  $PaCO_2$  should be maintained within the normal range during the Trendelenburg-pneumoperitoneum position. It has also been suggested that  $rSO_2$  measurements can best be assessed if patient's body position and  $PaCO_2$  are held constant.<sup>22</sup>

The  $rSO_2$  value from near-infrared spectroscopy reflects saturation in a mixture of 25% arterial, 70% venous and 5% capillary compartments. The changes in body position may alter the ratio of arterial and venous blood compartment in the cerebral circulation; therefore, the validity of  $rSO_2$  is questionable in this situation.

CBF- $CO_2$  reactivity represents the ability of cerebral vasculature to respond to changes in cerebral metabolic demands. In this study, the  $SjvO_2$ - $CO_2$  reactivity was higher than  $rSO_2$ - $CO_2$  reactivity in the supine position and Trendelenburg-pneumoperitoneum condition, respectively. We previously demonstrated that CBF- $CO_2$  reactivity measured by  $SjvO_2$  was preserved in the modest Trendelenburg position under pneumoperitoneum during sevoflurane anesthesia if  $PaCO_2$  was controlled.<sup>23</sup> Therefore, it is suggested that  $SjvO_2$  may represent the change of CBF in relation to the

change of  $PaCO_2$  more accurately than  $rSO_2$  during laparoscopic surgery. There is general agreement that  $rSO_2$  may be valuable as a trend monitor, but that it is less useful as an indicator of cerebral ischemia. Our results demonstrate that the validity of  $rSO_2$  is also questionable during Trendelenburg-pneumoperitoneum condition.

In this study,  $SjvO_2$ - $CO_2$  reactivity was significantly higher in the Trendelenburg-pneumoperitoneum condition compared to the supine position. This result means that the change of CBF according to the change of  $PaCO_2$  was greater in the Trendelenburg-pneumoperitoneum condition than in the supine position. Therefore, we suggested that it is necessary to control  $PaCO_2$  for the prevention of an increase of CBF during laparoscopic surgery.

There were some limitations in this study. First, we measured  $SjvO_2$  unilaterally and compared it with the average value of  $rSO_2$  from both sides. Secondly, the patients of the study were all American Society of Anesthesiologists physical status I or II without any cardiopulmonary diseases. This may limit the extrapolation of our results to patients with severe cardiopulmonary compromise. Lastly, intraoperative variables were measured at arbitrary time points without exact information on time dependent cardiopulmonary changes. Therefore, the optimal time points of evaluation when the patient is in the Trendelenburg position with  $CO_2$  pneumoperitoneum cannot be guaranteed.

In conclusion, there is little correlation between  $SjvO_2$  and  $rSO_2$  in the supine position and Trendelenburg-pneumoperitoneum condition. Therefore, both  $rSO_2$  and  $SjvO_2$  are not interchangeable values in this condition.

## ACKNOWLEDGEMENTS

This research was supported by Basic Science Research Program through the National Research Foundation of Korea (NRF) funded by the Ministry of Education, Science and Technology (NRF-2010-0022999).

## REFERENCES

1. Mottrie A, Van Migem P, De Naeyer G, Schatteman P, Carpentier P, Fonteyne E. Robot-assisted laparoscopic radical prostatectomy: oncologic and functional results of 184 cases. *Eur Urol* 2007;52: 746-50.
2. Fujii Y, Tanaka H, Tsuruoka S, Toyooka H, Amaha K. Middle cerebral arterial blood flow velocity increases during laparoscopic

- cholecystectomy. *Anesth Analg* 1994;78:80-3.
3. Huettemann E, Terborg C, Sakka SG, Petrat G, Schier F, Reinhart K. Preserved CO(2) reactivity and increase in middle cerebral arterial blood flow velocity during laparoscopic surgery in children. *Anesth Analg* 2002;94:255-8.
  4. Smythe PR, Samra SK. Monitors of cerebral oxygenation. *Anesthesiol Clin North America* 2002;20:293-313.
  5. Macmillan CS, Andrews PJ. Cerebrovenous oxygen saturation monitoring: practical considerations and clinical relevance. *Intensive Care Med* 2000;26:1028-36.
  6. Tobias JD. Cerebral oxygenation monitoring: near-infrared spectroscopy. *Expert Rev Med Devices* 2006;3:235-43.
  7. Casati A, Spreafico E, Putzu M, Fanelli G. New technology for noninvasive brain monitoring: continuous cerebral oximetry. *Minerva Anesthesiol* 2006;72:605-25.
  8. Yao FS, Tseng CC, Ho CY, Levin SK, Illner P. Cerebral oxygen desaturation is associated with early postoperative neuropsychological dysfunction in patients undergoing cardiac surgery. *J Cardiothorac Vasc Anesth* 2004;18:552-8.
  9. Nagdyman N, Ewert P, Peters B, Miera O, Fleck T, Berger F. Comparison of different near-infrared spectroscopic cerebral oxygenation indices with central venous and jugular venous oxygenation saturation in children. *Paediatr Anaesth* 2008;18:160-6.
  10. Leyvi G, Bello R, Wasnick JD, Plestis K. Assessment of cerebral oxygen balance during deep hypothermic circulatory arrest by continuous jugular bulb venous saturation and near-infrared spectroscopy. *J Cardiothorac Vasc Anesth* 2006;20:826-33.
  11. Nagdyman N, Fleck T, Schubert S, Ewert P, Peters B, Lange PE, et al. Comparison between cerebral tissue oxygenation index measured by near-infrared spectroscopy and venous jugular bulb saturation in children. *Intensive Care Med* 2005;31:846-50.
  12. Barnhart HX, Haber M, Song J. Overall concordance correlation coefficient for evaluating agreement among multiple observers. *Biometrics* 2002;58:1020-7.
  13. Bland JM, Altman DG. Statistical methods for assessing agreement between two methods of clinical measurement. *Lancet* 1986;1:307-10.
  14. Kim MB, Ward DS, Cartwright CR, Kolano J, Chlebowski S, Henson LC. Estimation of jugular venous O2 saturation from cerebral oximetry or arterial O2 saturation during isocapnic hypoxia. *J Clin Monit Comput* 2000;16:191-9.
  15. Brown R, Wright G, Royston D. A comparison of two systems for assessing cerebral venous oxyhaemoglobin saturation during cardiopulmonary bypass in humans. *Anaesthesia* 1993;48:697-700.
  16. Fearn SJ, Chant HJ, Picton AJ, Mortimer AJ, McCollum CN. The contribution of extracranial blood oxygenation on near-infrared spectroscopy during carotid endarterectomy. *Anaesthesia* 1997;52:704-5.
  17. Knirsch W, Stutz K, Kretschmar O, Tomaske M, Balmer C, Schmitz A, et al. Regional cerebral oxygenation by NIRS does not correlate with central or jugular venous oxygen saturation during interventional catheterisation in children. *Acta Anaesthesiol Scand* 2008;52:1370-4.
  18. Dullenkopf A, Frey B, Baenziger O, Gerber A, Weiss M. Measurement of cerebral oxygenation state in anaesthetized children using the INVOS 5100 cerebral oximeter. *Paediatr Anaesth* 2003;13:384-91.
  19. Yoshitani K, Kawaguchi M, Tatsumi K, Kitaguchi K, Furuya H. A comparison of the INVOS 4100 and the NIRO 300 near-infrared spectrophotometers. *Anesth Analg* 2002;94:586-90.
  20. Lee JR, Lee PB, Do SH, Jeon YT, Lee JM, Hwang JY, et al. The effect of gynaecological laparoscopic surgery on cerebral oxygenation. *J Int Med Res* 2006;34:531-6.
  21. Park EY, Koo BN, Min KT, Nam SH. The effect of pneumoperitoneum in the steep Trendelenburg position on cerebral oxygenation. *Acta Anaesthesiol Scand* 2009;53:895-9.
  22. Pollard V, Prough DS, DeMelo AE, Deyo DJ, Uchida T, Widman R. The influence of carbon dioxide and body position on near-infrared spectroscopic assessment of cerebral hemoglobin oxygen saturation. *Anesth Analg* 1996;82:278-87.
  23. Choi SH, Lee SJ, Rha KH, Shin SK, Oh YJ. The effect of pneumoperitoneum and Trendelenburg position on acute cerebral blood flow-carbon dioxide reactivity under sevoflurane anaesthesia. *Anaesthesia* 2008;63:1314-8.